


WARNING!

The Rotation Lock is not locked with a handle!

To Lock the Rotation Cushion:

- Turn the handle (marked "A" in the photo) down to the six o'clock position to level the cushion
- Push the Mechlok switch lever (marked "B" in the photo) in towards the patient to lock the cushion

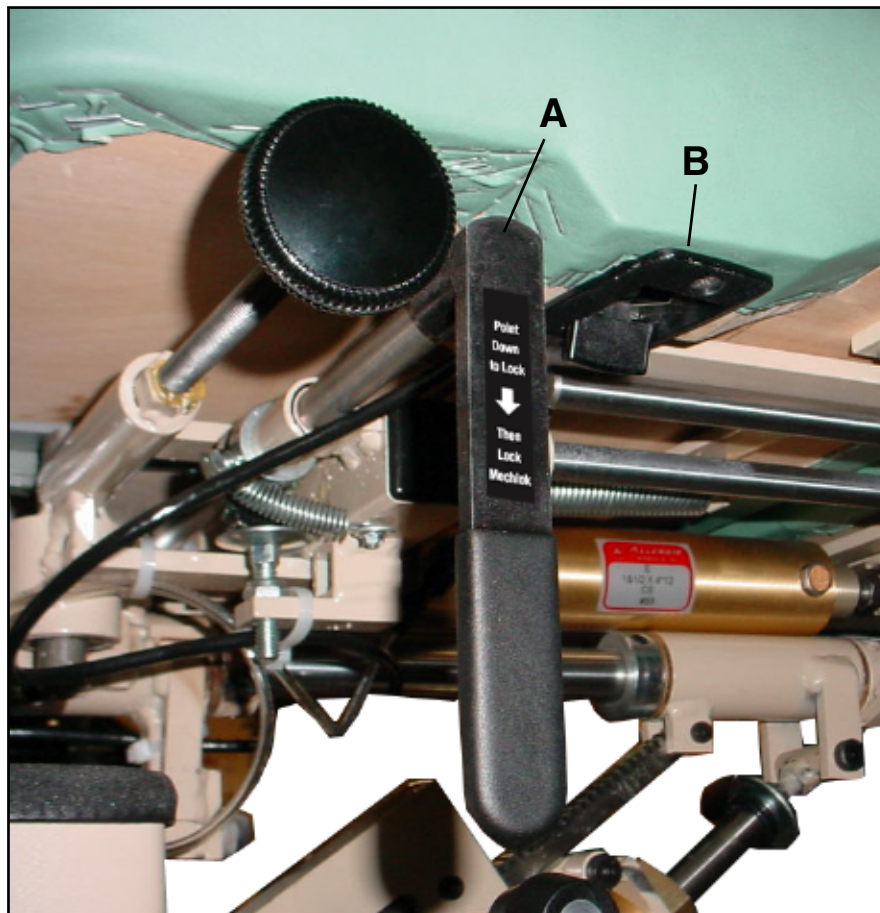


Hill Laboratories
COMPANY

3 Bacton Hill, Frazer, PA 19355 • 610-644-2867 • fax 610-647-6297 www.hilllabs.com

af_rotation_lock_warning.qxd 2/05